


OBTA: ON IALT-F1/BB=601

File Dynamics, Inc.

DPF

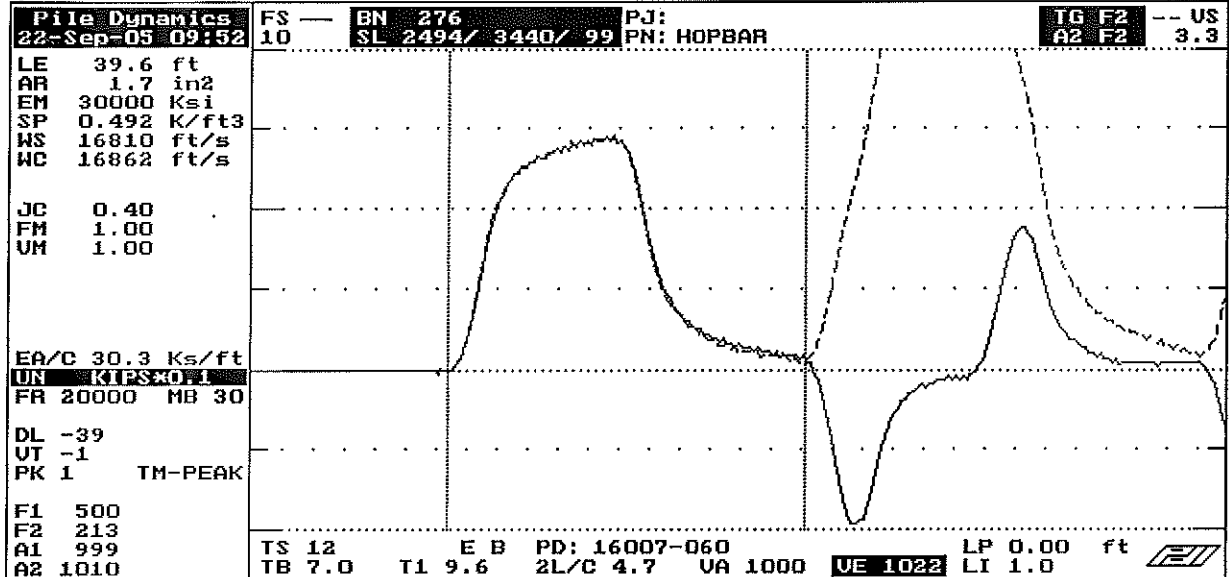

<b>ACCEPT</b> SQ-OFF FL-OFF PR-OFF   contact File Dynamics USA with your questions tel USA - 216 - 831- 6131 fax USA - 216 - 831- 0916	UMX= 4.7 FMX= 72 AMX= 149 EMX= 0.3 MEX= 141 FUP= 0.99 ACCELEROMETER CALIBRATION N.I.S.T. Traceable SERIAL NUMBER: 16007 CALIBRATION FACTOR: 1010 G/V PAK <del>(#5000)</del> : _____ DATE: 22-Sep-05 PDA OPERATOR: <i>John Han</i> OP: FRED Ivar: 4.051
--	---

<-AT:PIEZORESISTIVE

AT:PIEZOELECTRIC->