


QBTA: ON [ALT-F1/BB=60]

File Dynamics, Inc.

DPF

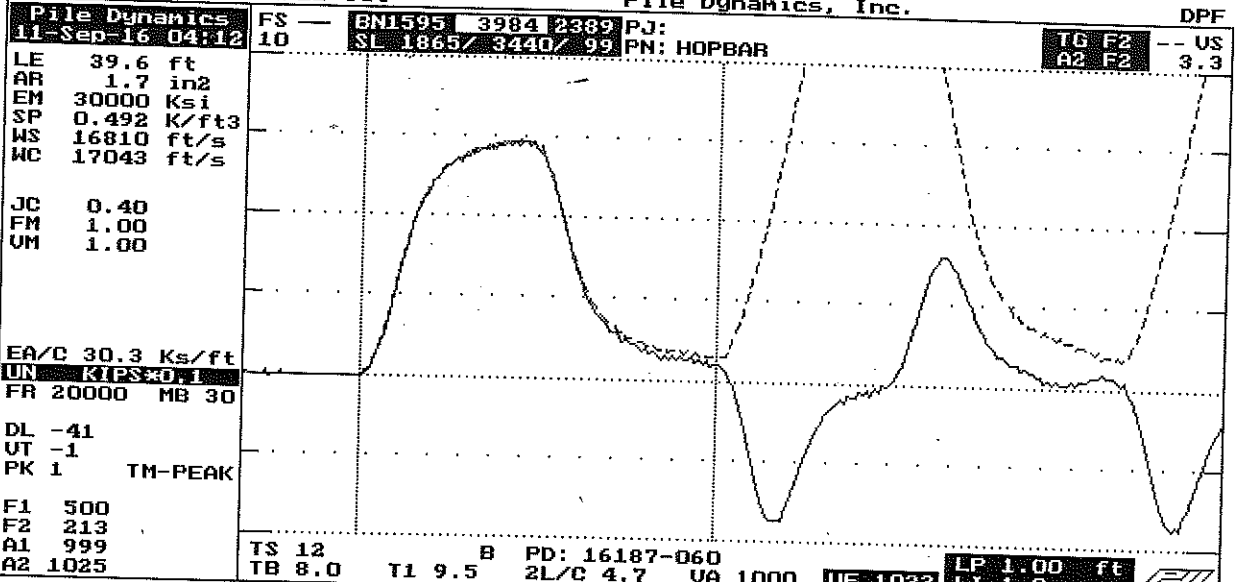

ACCEPT SQ-OFF FL-OFF PR-OFF



contact File Dynamics USA
with your questions
tel USA - 216 - 831- 6131
fax USA - 216 - 831- 0916

UMX= 4.7 FMX= 74 AMX= 139
EMX= 0.4 MEX= 145 FVP= 0.99

ACCELEROMETER CALIBRATION N.I.S.T. Traceable

SERIAL NUMBER: 16187

CALIBRATION FACTOR: 1025 %/V

PAK (*5000): 1025 %/V DATE: 15SEPT16

PDA OPERATOR: *[Signature]*

<-AT:PIEZORESISTIVE

OP: laine [ver:4.05]

AT:PIEZOELECTRIC->

Smart Sensor

Smart Chip Programmed By A.M.W. on 15SEPT16 CRC Value 0758