


QBTA: ON [ALT-F1/BB=60]

File Dynamics, Inc.

DPF

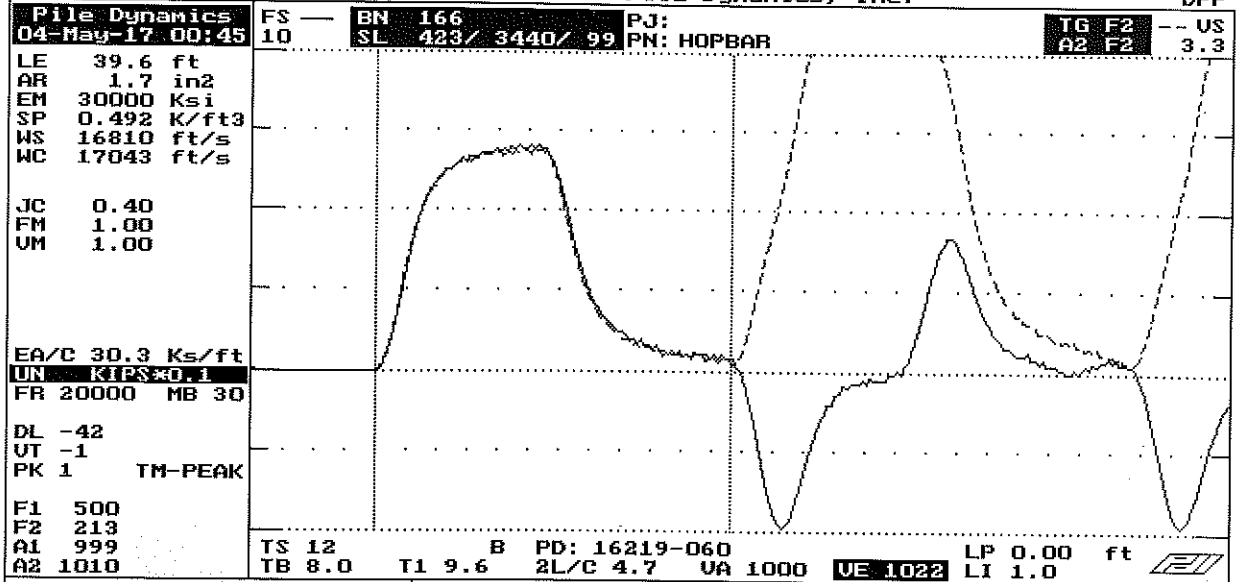

UMX= 4.5 FMX= 70 AMX= 149
EMX= 0.3 MEX= 137 FUP= 1.01

ACCELEROMETER CALIBRATION N.I.S.T. Traceable
SERIAL NUMBER: 16219
CALIBRATION FACTOR: 1010 g/v
PAK (*5000): DATE: 4 MAY 17
PDA OPERATOR: [Signature]

<-AT:PIEZORESISTIVE OP: laine [ver:4.05] AT:PIEZOELECTRIC->