


QBTA: ON [ALT-F1/BB=60]

File Dynamics, Inc.

DPF

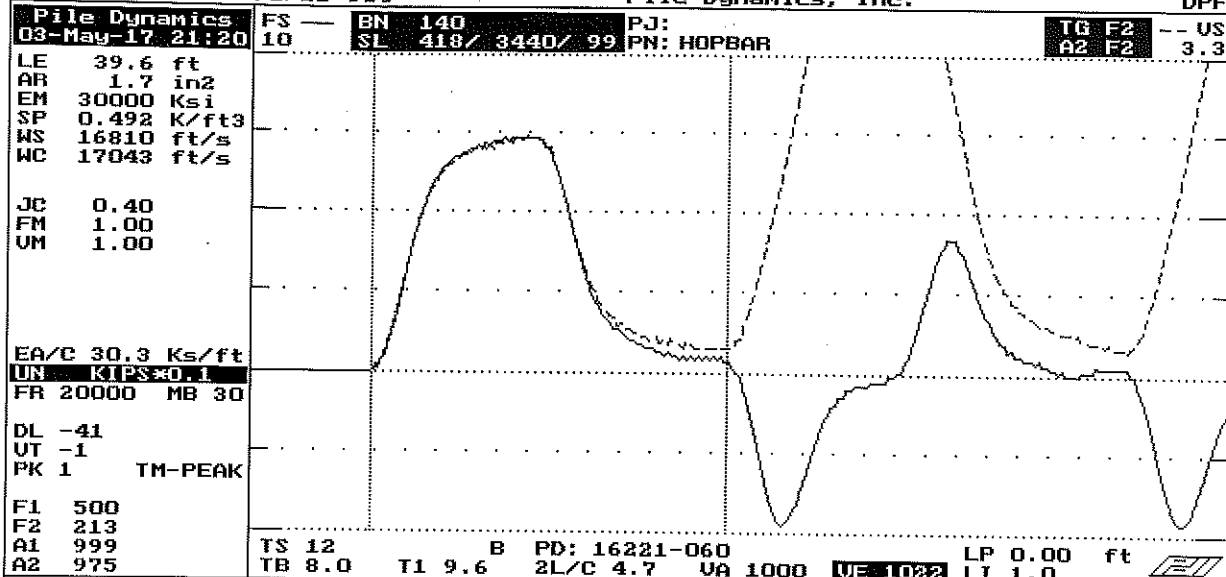

ACCEPT SQ-OFF FL-OFF PR-OFF

UMX= 4.7 FMX= 74 AMX= 139  
 EMX= 0.3 MEX= 145 FUP= 1.01



contact File Dynamics USA  
 with your questions  
 tel USA - 216 - 831- 6131  
 fax USA - 216 - 831- 0916

ACCELEROMETER CALIBRATION N.I.S.T. Traceable

SERIAL NUMBER: 16221

CALIBRATION FACTOR: 975 %

PAK-(\*5888): \_\_\_\_\_ DATE: 4 MAY 17

PDA OPERATOR: [Signature]

<-AT:PIEZORESISTIVE

OP: laine lver:4.051

AT:PIEZOELECTRIC->