


OBTA: ON [ALT-F1/BB=60]

Pile Dynamics, Inc.

DPF

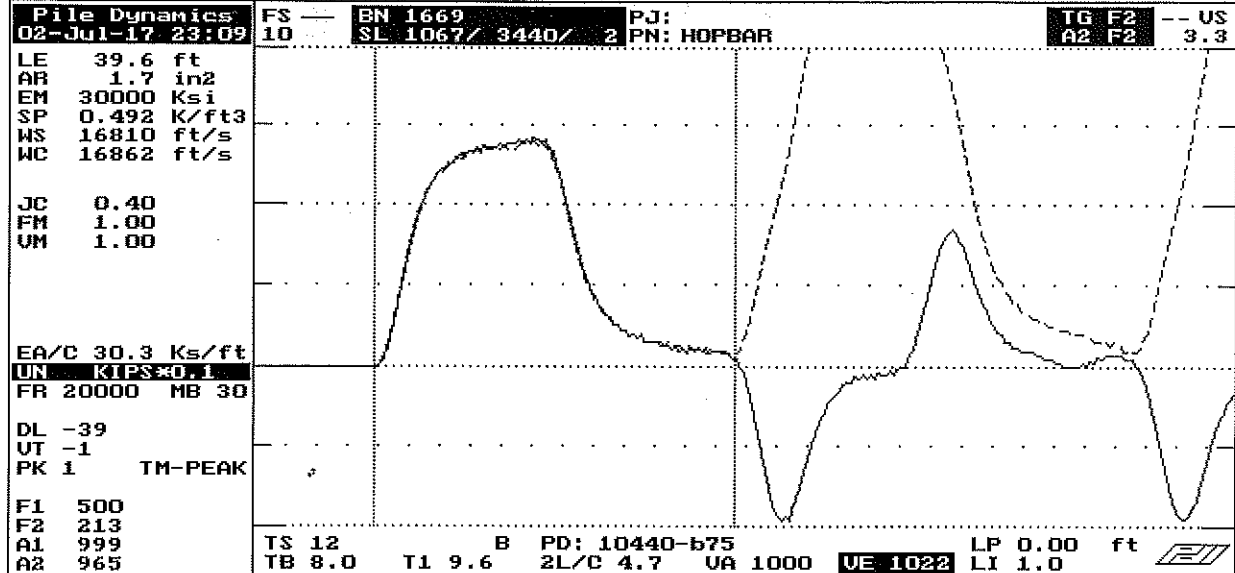

ACCEPT SQ-OFF FL-OFF PR-OFF	UMX= 4.5 FMX= 71 AMX= 159
	EMX= 0.3 MEX= 139 FVP= 1.00
<p>contact Pile Dynamics USA with your questions tel USA - 216 - 831- 6131 fax USA - 216 - 831- 0916</p>	ACCELEROMETER CALIBRATION N.I.S.T. Traceable
	SERIAL NUMBER: 10440
	CALIBRATION FACTOR: 965 %
	PAK <5000>: DATE: 10 July 17
	PDA OPERATOR: <i>[Signature]</i>

<-AT:PIEZORESISTIVE

OP: Iaine [ver:4.05]

AT:PIEZOELECTRIC->