



QBTA: ON [ALT-F1/BB=60]

File Dynamics, Inc.

DPF

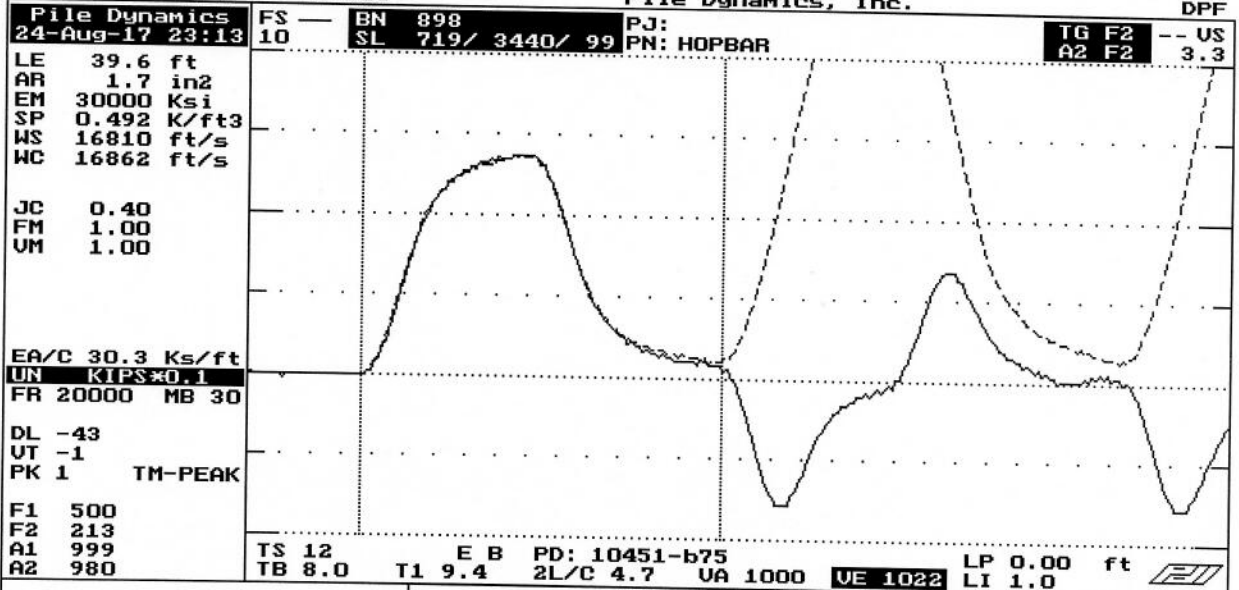

ACCEPT SQ-OFF FL-OFF PR-OFF	UMX= 4.5 FMX= 69 AMX= 129	
	EMX= 0.3 MEX= 135 FVP= 1.01	
 <p>contact File Dynamics USA with your questions tel USA - 216 - 831- 6131 fax USA - 216 - 831- 0916</p>	ACCELEROMETER CALIBRATION N.I.S.T. Traceable	
	SERIAL NUMBER: 10451	
	CALIBRATION FACTOR: 980 g/v	
	PAK (*5000): _____ DATE: 28 AUG 17	
	PDA OPERATOR: <i>[Signature]</i>	
<-AT:PIEZORESISTIVE	OP: laine [ver:4.05]	AT:PIEZOELECTRIC->