



QBTA: ON [ALT-F1/BB=60]

File Dynamics, Inc.

DPF

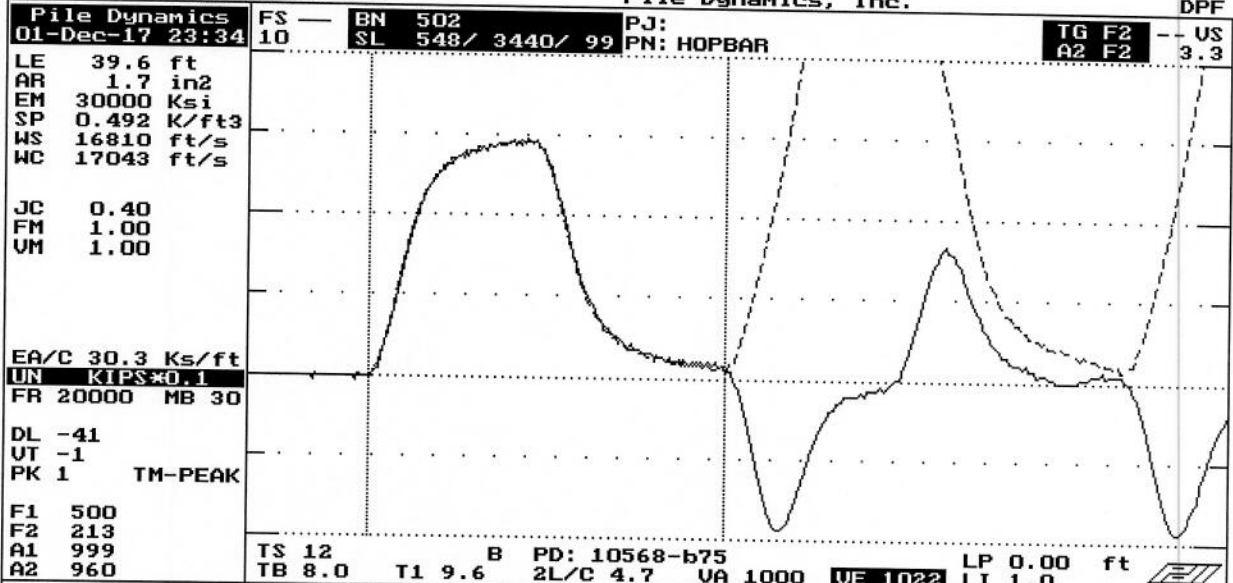

ACCEPT SQ-OFF FL-OFF PR-OFF	UMX= 4.7 FMX= 74 AMX= 159
	EMX= 0.3 MEX= 145 FUP= 1.00
 <p>contact File Dynamics USA with your questions tel USA - 216 - 831- 6131 fax USA - 216 - 831- 0916</p>	ACCELEROMETER CALIBRATION N.I.S.T. Traceable
	SERIAL NUMBER: 10568
	CALIBRATION FACTOR: 960 %/V
	PAK (*5000): DATE: 8 DEC 17
	PDA OPERATOR: <i>[Signature]</i>
<-AT:PIEZORESISTIVE	OP: laine [ver:4.05]
	AT:PIEZOELECTRIC->