


QBTA: ON [ALT-F1/BB=60]

Pile Dynamics, Inc.

DPF

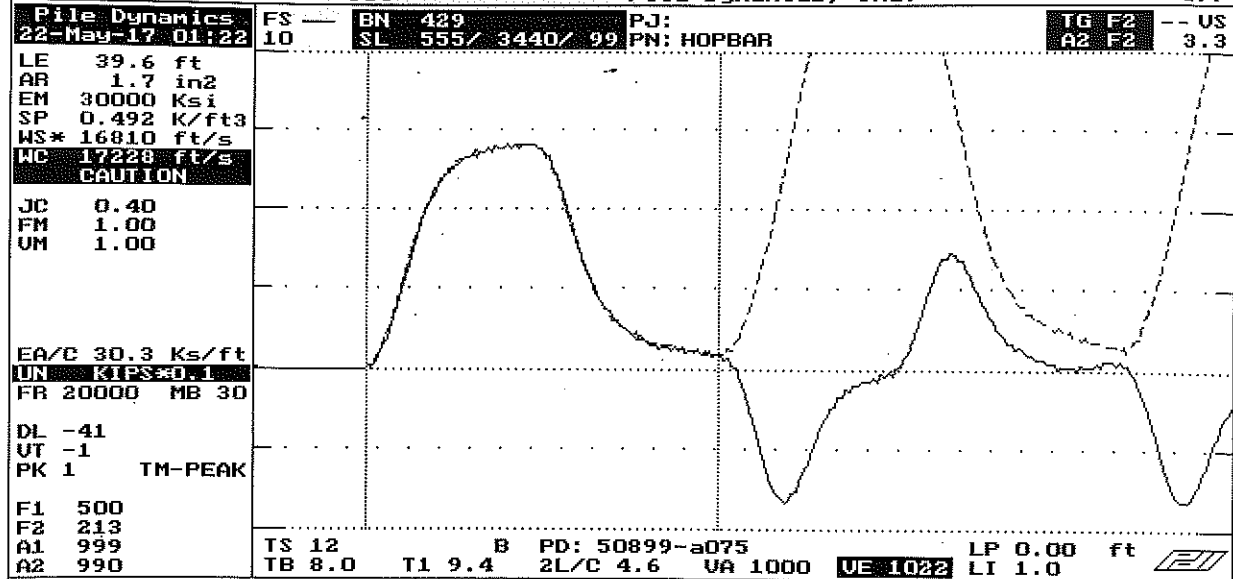

contact Pile Dynamics USA  
with your questions  
tel USA - 216 - 831- 6131  
fax USA - 216 - 831- 0916

ACCELEROMETER CALIBRATION N.I.S.T. Traceable  
 SERIAL NUMBER: 50899  
 CALIBRATION FACTOR: 990 G/V  
 PAK (\*5000): DATE: 23 MAY 17  
 PDA OPERATOR: *Da*

<-AT:PIEZORESISTIVE

OP: Iaine [ver:4.05]

AT:PIEZOELECTRIC->

Smart Sensor

Smart Chip Programmed By A.M.W. on 23 MAY 17 CRC Value 4640