


OBTA: ON [ALT-F1/BB=60]

File Dynamics, Inc.

DPF

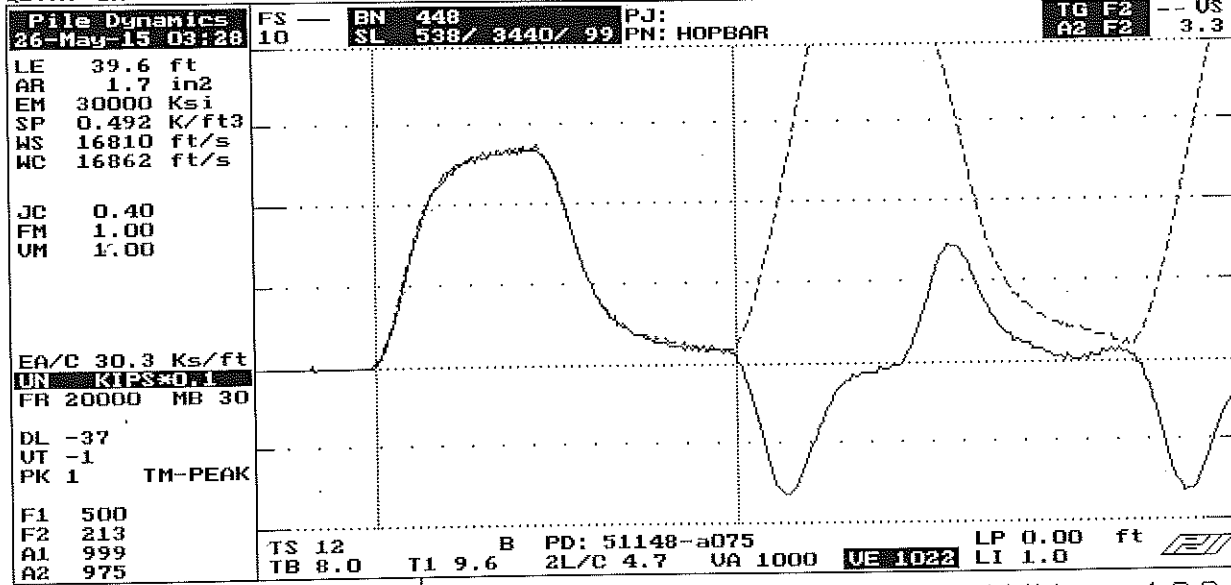

ACCEPT SQ-OFF FL-OFF PR-OFF

UMX= 4.4 FMX= 67 AMX= 139  
 EMX= 0.3 MEX= 131 FUP= 0.98



contact File Dynamics USA  
 with your questions  
 tel USA - 216 - 831- 6131  
 fax USA - 216 - 831- 0916

ACCELEROMETER CALIBRATION N.I.S.T. Traceable  
 SERIAL NUMBER: 51148  
 CALIBRATION FACTOR: 975%  
 PAK (\*5000): DATE: 26MAY15  
 PDA OPERATOR: *M. W. W.*  
 OP: laine fver:4.051

<-AT:PIEZORESISTIVE

ATPIEZOELECTRIC->

Smart Sensor

Smart Chip Programmed By *M.W.* on *26MAY15* CRC Value *5392*