


QBTA: ON IALT-F1/BB=601

File Dynamics, Inc.

DPF

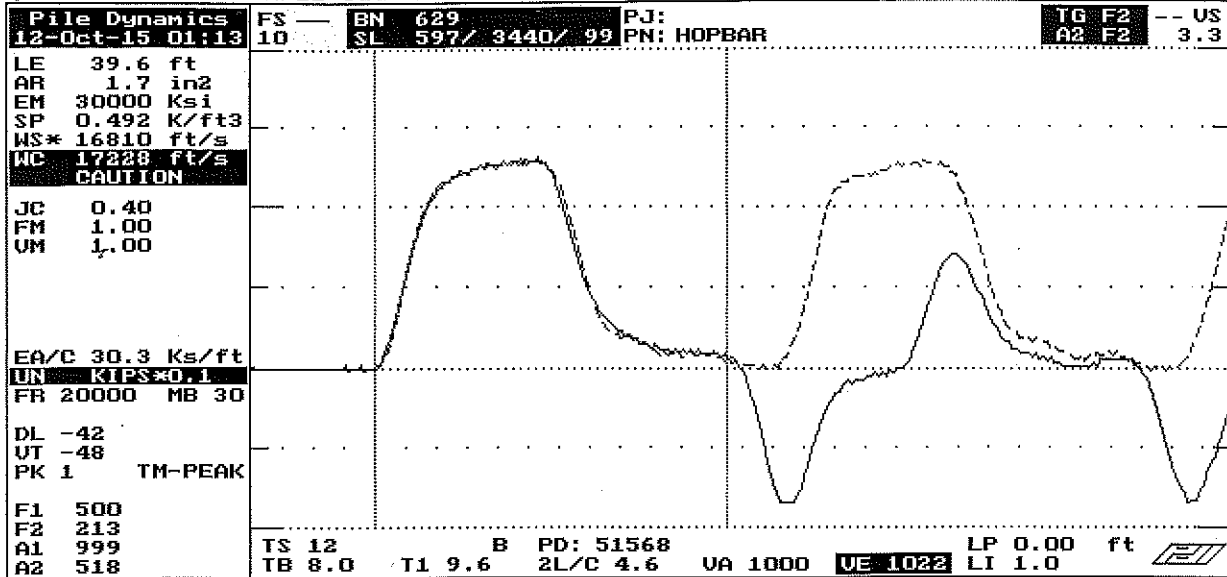

VMX= 2.1 FMX= 66 AMX= 129
 EMX= 0.5 MEX= 129 FVP= 0.99
 ACCELEROMETER CALIBRATION N.I.S.T. Traceable
 SERIAL NUMBER: 51568
 CALIBRATION FACTOR: 1036%
 PAK (*5000): DATE: 1300T15
 PDA OPERATOR: *DAF*
 <-AT:PIEZORESISTIVE OP: Iaine [ver:4.05] AT:PIEZOELECTRIC->