


QBTA: ON [ALT-F1/BB=60]

File Dynamics, Inc.

DPF

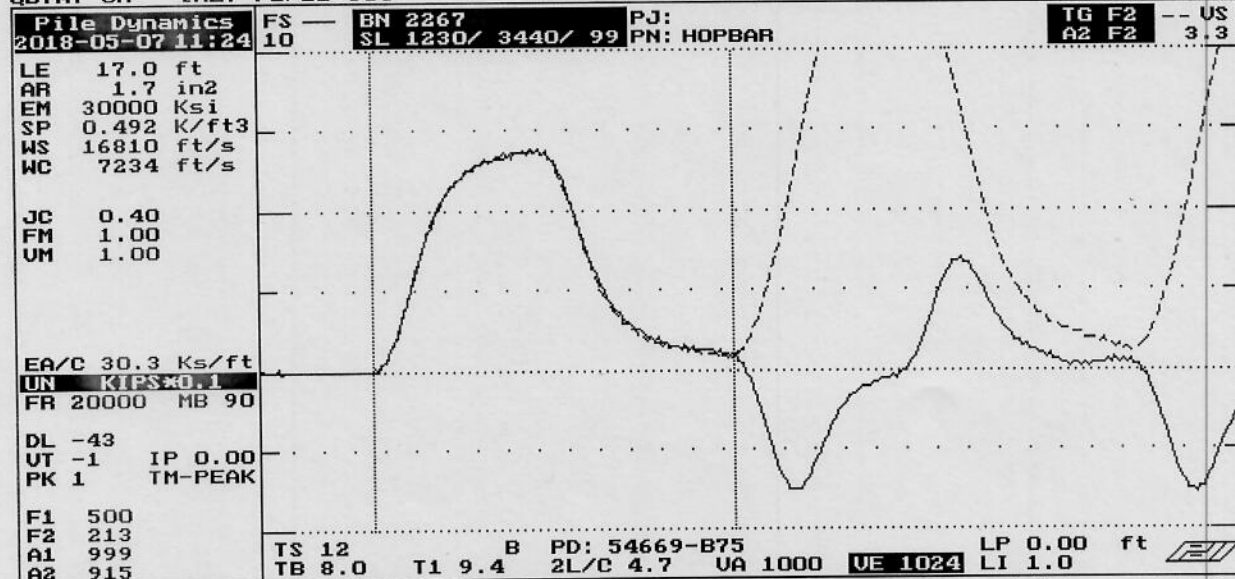

ACCEPT SQ-OFF FL-OFF PR-OFF	UMX= 4.4	FMX= 69	AMX= 129
	EMX= 0.3	MEX= 135	FUP= 1.00
ACCEPT	ACCELEROMETER CALIBRATION N.I.S.T. Traceable		
	SERIAL NUMBER:	54669	
	CALIBRATION FACTOR:	915 g/v	
	PAK (*5000):	DATE: 7 MAY 18	
	PDA OPERATOR:	[Signature]	

<-AT:PIEZORESISTIVE OP: laine [ver:5.01] AT:PIEZOELECTRIC->

Smart Sensor

Smart Chip Programmed By Z.W. on 7 MAY 18 CRC Value 962C