



QBTA: ON [ALT-F1/BB=60]

Pile Dynamics, Inc.

DPF

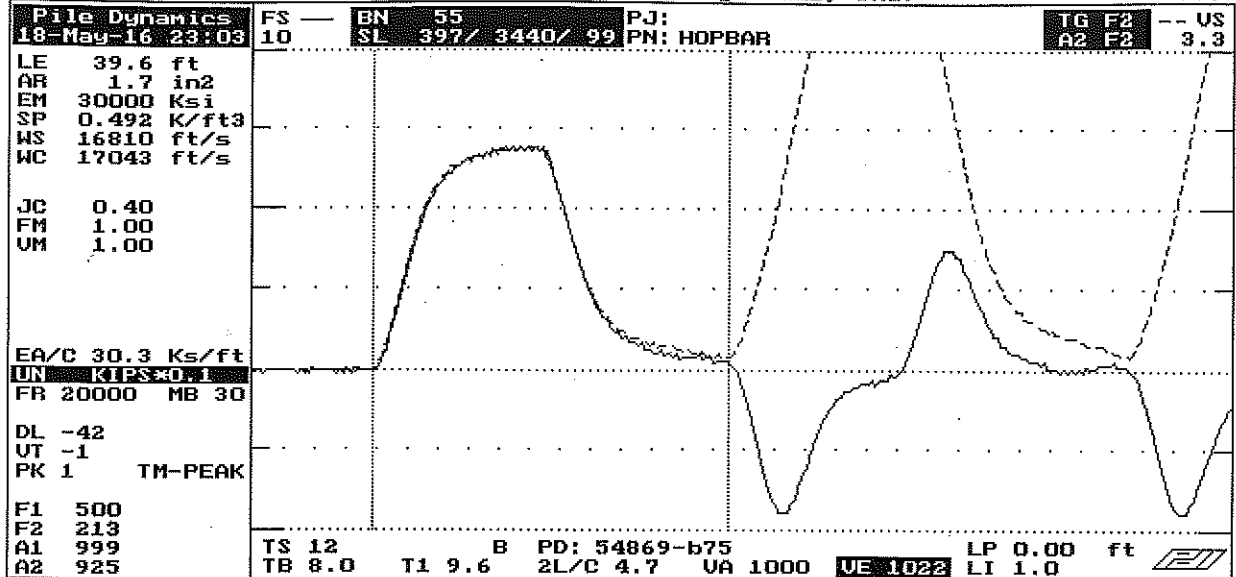

ACCEPT SQ-OFF FL-OFF PR-OFF	UMX= 4.5	FMX= 69	AMX= 139
	EMX= 0.3	MEX= 135	FVP= 1.00
 <p>contact Pile Dynamics USA with your questions tel USA - 216 - 831- 6131 fax USA - 216 - 831- 0916</p>	ACCELEROMETER CALIBRATION		N.I.S.T. Traceable
	SERIAL NUMBER:	54869	
	CALIBRATION FACTOR:	925%	
	PAK (*5000):	DATE: 19 MAY 16	
	PDA OPERATOR:	[Signature]	
←-AT:PIEZORESISTIVE		OP: Iaine [ver:4.05]	AT:PIEZOELECTRIC→

Smart Sensor

Smart Chip Programmed By Z.M.W. on 19 MAY 16 CRC Value 5F65