


QBTA: ON [ALT-F1/BB=60]

File Dynamics, Inc.

DPF

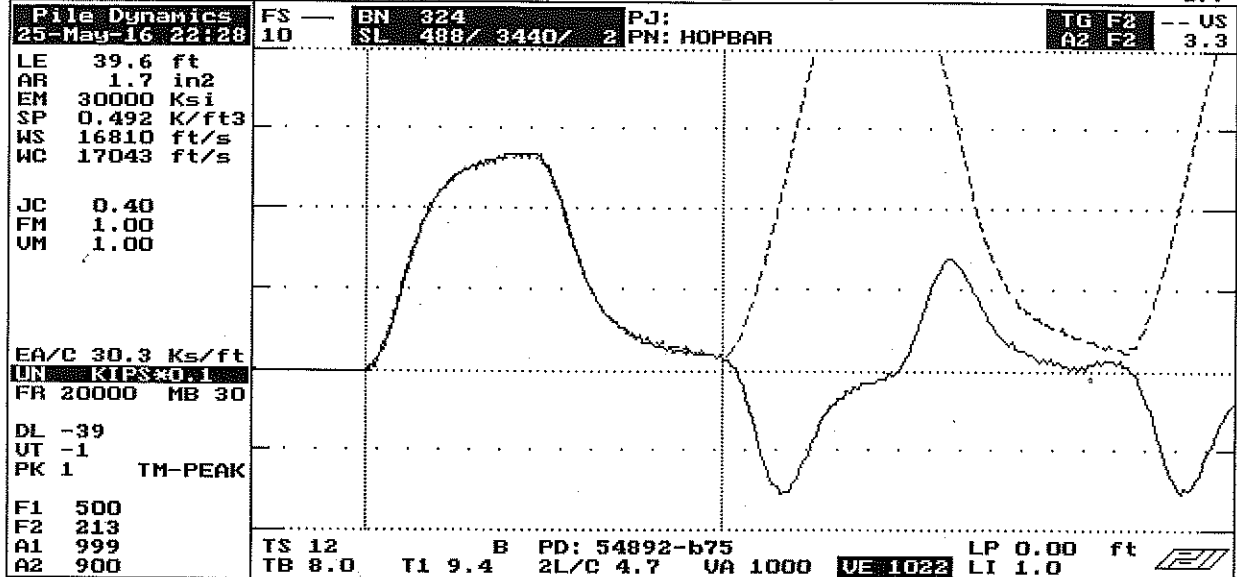

ACCERT SQ-OFF FL-OFF PR-OFF	UMX= 4.3	FMX= 68	AMX= 129
	EMX= 0.3	MEX= 133	FVP= 1.02
	ACCELEROMETER CALIBRATION N.I.S.T. Traceable		
contact File Dynamics USA with your questions tel USA - 216 - 831- 6131 fax USA - 216 - 831- 0916	SERIAL NUMBER: <u>54892</u>		
	CALIBRATION FACTOR: <u>900%/V</u>		
	PAK (*5000): _____ DATE: _____		
	PDA OPERATOR: <u>Ja</u>		
<-AT:PIEZORESISTIVE	OP: Iaine [ver:4.05]	AT:PIEZOELECTRIC->	

Smart Sensor

Smart Chip Programmed By A.M.W. on _____ CRC Value 3076