


QBTA: ON [ALT-F1/BB=60]

File Dynamics, Inc.

DPF

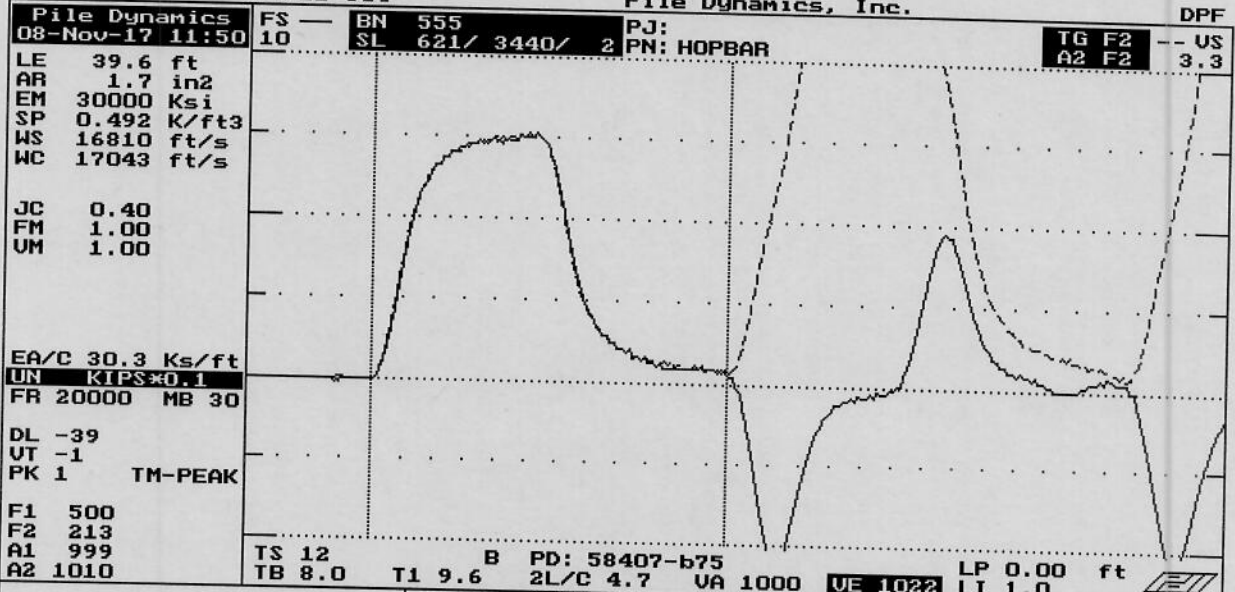

ACCEPT SQ-OFF FL-OFF PR-OFF	VMX= 4.9	FMX= 76	AMX= 169
	EMX= 0.4	MEX= 149	FVP= 1.00
	ACCELEROMETER CALIBRATION N.I.S.T. Traceable		
contact File Dynamics USA with your questions tel USA - 216 - 831- 6131 fax USA - 216 - 831- 0916	SERIAL NUMBER: 58407		
	CALIBRATION FACTOR: 1010 G/V		
	PAK (*5000): _____ DATE: 8 NOV 17		
	PDA OPERATOR: <i>[Signature]</i>		
<-AT:PIEZORESISTIVE	OP: laine [ver:4.05]	AT:PIEZOELECTRIC->	

Smart Sensor

Smart Chip Programmed By J.M.W. on 8 NOV 17 CRC Value 6E19